

Alloyed steel — Determination of manganese — Potentiometric and visual titration method

ICS 77.140.20

National foreword

This British Standard is the UK implementation of ISO 18632:2010.

The UK participation in its preparation was entrusted to Technical Committee ISE/102, Methods of Chemical Analysis for Iron and Steel.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2010

© BSI 2010

ISBN 978 0 580 66234 8

Amendments/corrigenda issued since publication

Date	Comments

INTERNATIONAL STANDARD

BS ISO 18632:2010

ISO
18632

First edition
2010-06-15

Alloyed steel — Determination of manganese — Potentiometric and visual titration method

*Aciers alliés — Détermination de la teneur en manganèse — Méthodes
de titration visuelle et potentiométrique*



Reference number
ISO 18632:2010(E)

© ISO 2010

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2010

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope.....	1
2 Normative references.....	1
3 Principle.....	1
4 Reagents.....	1
5 Apparatus.....	4
6 Sampling and samples.....	4
7 Procedure.....	4
8 Expression of results.....	5
9 Test report.....	7
Annex A (informative) Additional information on the international cooperative test.....	8
Annex B (informative) Graphical representation of precision data	10
Bibliography.....	11

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 18632 was prepared by Technical Committee ISO/TC 17, *Steel*, Subcommittee SC 1, *Methods of determination of chemical composition*.

Alloyed steel — Determination of manganese — Potentiometric and visual titration method

1 Scope

This International Standard specifies a potentiometric or visual titration method for the determination of the mass fraction of manganese in alloyed steels. The method is applicable to mass fractions of manganese between 2 % and 25 %. Vanadium and cerium interfere with the measurement. If the mass fraction of cerium in the sample is less than 0,01 %, or the mass fraction of vanadium in the sample is less than 0,005 %, the interference is negligible. If the mass fraction of cerium in the sample is greater than 0,01 %, or the mass fraction of vanadium in the sample is greater than 0,005 %, a theoretical correction is necessary.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 648, *Laboratory glassware — Single-volume pipettes*

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 4942, *Steel and iron — Determination of vanadium content — N-BPHA spectrophotometric method*

ISO 4947:1986, *Steel and cast iron — Determination of vanadium content — Potentiometric titration method*

ISO 9647:1989, *Steel and iron — Determination of vanadium content — Flame atomic absorption spectrometric method*

ISO 14284:1996, *Steel and iron — Sampling and preparation of samples for the determination of chemical composition*

3 Principle

Dissolution of a test portion in appropriate acids. Addition of phosphoric acid. Oxidation of manganese to manganese(III) in phosphoric acid medium with ammonium nitrate. Visual titration of manganese(III) with ferroammoniumdisulfate standard solution with N-phenylanthranilic acid as the indicator. Alternatively, potentiometric titration with ferroammoniumdisulfate standard solution. If the sample contains vanadium and cerium, the mass fraction of manganese shall be corrected.

4 Reagents

During the analysis, use only reagents of recognized analytical grade and only grade 2 water as specified in ISO 3696.

4.1 Ammonium nitrate, NH_4NO_3 .

4.2 Urea.

4.3 Phosphoric acid, ρ approximately 1,69 g/ml.

4.4 Nitric acid, ρ approximately 1,42 g/ml.

4.5 Hydrochloric acid, ρ approximately 1,19 g/ml.

4.6 Sulfuric acid, diluted 1+3.

4.7 Sulfuric acid, diluted 5+95.

4.8 N-phenylanthranilic acid solution, $\text{C}_6\text{H}_5\text{NHC}_6\text{H}_4\text{COOH}$, approximately 2 g/l.

Dissolve 0,20 g of N-phenylanthranilic acid and 0,20 g of sodium carbonate in 100 ml of water and filter.

4.9 Potassium dichromate solution, 0,002 50 mol/l.

Weigh 0,735 5 g of high-purity potassium dichromate which shall be previously dried at 150 °C for at least 2 h and cooled in a desiccator. Put the weighed mass in a 250 ml beaker and dissolve it in water. Transfer the solution quantitatively into a 1 000 ml one-mark volumetric flask, dilute to the mark with water and mix.

4.10 Manganese standard solution, corresponding to 1,00 g of Mn per litre.

Weigh, to the nearest 0,1 mg, 1,000 g of pure manganese metal [purity W 99,9 % (mass fraction)]. Place it in a 250 ml beaker and add 40 ml of hydrochloric acid (4.5). Cover with a watch glass and heat gently until complete dissolution. Cool and transfer the solution quantitatively to a 1 000 ml one-mark volumetric flask, dilute to the mark with water and mix. 1 ml of this standard solution contains 1,00 mg of Mn.

4.11 Ferroammoniumdisulfate solution, standard volumetric solution, 0,015 mol/l.

4.11.1 Preparation of the solution.

Dissolve 5,9 g of ferroammoniumdisulfate $[(\text{NH}_4)\text{Fe}(\text{SO}_4)_2 \cdot 6\text{H}_2\text{O}]$ in 1 000 ml of sulfuric acid (4.7) and mix.

4.11.2 Standardization of the solution (to be carried out just before use).

4.11.2.1 Visual titration method.

4.11.2.1.1 Titration.

Transfer three portions of 20,00 ml of the potassium dichromate solution (4.9) to three 250 ml conical flasks.

Add 20 ml of sulfuric acid (4.6), 5 ml of phosphoric acid (4.3). Add water up to a volume of approximately 150 ml. Proceed as specified in 7.2.2.1.

Calculate the mean of the three values of the ferroammoniumdisulfate solution volume, V_1 . The difference between the values should not exceed 0,05 ml.

4.11.2.1.2 Correction for N-phenylanthranilic acid.

Transfer three portions of 5,00 ml of the potassium dichromate solution (4.9) to three 250 ml conical flasks. Add 20 ml of sulfuric acid (4.6) and 5 ml of phosphoric acid (4.3). Titrate the solution with the ferroammoniumdisulfate solution (4.11.1) until the end point is approached¹⁾. Add 2 drops of N-phenylanthranilic acid solution (4.8), continue the titration until disappearance of the purplish red color and

1) The purplish red colour of the solution becomes light.

record the volume added. Add 5 ml more of potassium dichromate solution (4.9), titrate with the ferroammoniumdisulfate solution (4.11.1) until the end point and record the volume added again. The mean of the differences between the volumes of the two titrations is the corrected value of V_0 .

4.11.2.1.3 Calculation.

The corresponding concentration, c , in moles per litre (mol/l), of the ferroammoniumdisulfate solution (4.11.1) is given by the equation:

$$c = \frac{0,015\,00 \times 20,00}{V_1 - V_0}$$

where

V_1 is the mean volume, in millilitres, of the ferroammoniumdisulfate solution (4.11.1) added;

V_0 is the mean volume, in millilitres, of the ferroammoniumdisulfate solution (4.11.1) added for correction of N-phenylanthranilic acid.

4.11.2.2 Potentiometric titration method.

4.11.2.2.1 Titration.

Transfer three portions of 20,00 ml of the manganese standard solution (4.10) to three 300 ml conical flasks. Add 15 ml of phosphoric acid (4.3). Heat until the surface of the solution calms down²⁾ and white fumes are just given off (controlling the temperature from 200 °C to 240 °C). Remove the flask from the heater, add 2 g of ammonium nitrate (4.1) immediately and shake the conical flask to remove nitrogen oxide. Nitrogen oxide must be eliminated thoroughly by blowing with a pipette or by adding 0,5 g to 1,0 g of urea (4.2). Wait for 1 min to 2 min. Cool the solution to 80 °C to 100 °C.

Transfer the solution to a 400 ml beaker. Add 60 ml of sulfuric acid (4.7) and mix. Make up the volume to approximately 150 ml and cool to room temperature.

Proceed as specified in 7.2.2.2.

Calculate the mean of the three values of the ferroammoniumdisulfate solution volume, V_2 . The difference between the values should not exceed 0,05 ml.

4.11.2.2.2 Calculation.

The corresponding concentration, c_1 , in moles per litre, of the ferroammoniumdisulfate solution (4.11.1) is given by the equation:

$$c_1 = \frac{1,00 \times 20,00}{54,94 \times V_2}$$

where

V_2 is the mean volume, in millilitres, of the ferroammoniumdisulfate solution (4.11.1) required to titrate the manganese solution;

54,94 is the molar mass, in grams per mole, of manganese.

2) A stage where no bubble is observed on the surface of the solution.

5 Apparatus

All volumetric glassware shall be class A, in accordance with ISO 648 or ISO 1042, as appropriate. Ordinary laboratory apparatus shall be used, and also a potentiometric titration device, consisting of

- a) an indicator electrode, of bright platinum, which shall be kept in a clean, highly polished condition, and
- b) a reference electrode, of silver/silver chloride, calomel or mercury(I) sulfate

NOTE A redox electrode can also be used.

6 Sampling and samples

Carry out sampling in accordance with ISO 14284 or appropriate national standards for steel.

7 Procedure

7.1 Test portion

Weigh, to the nearest 0,000 1 g, a test portion of the sample in accordance with Table 1.

Table 1 — Test portion

Expected mass fraction of manganese %	Mass of test portion g
2 to 5	0,5
5 to 15	0,20
15 to 25	0,10

7.2 Determination

7.2.1 Preparation of the test solution

Transfer the test portion (7.1) to a 300 ml conical flask. Add 15 ml of phosphoric acid (4.3) [first add 15 ml of *aqua regia*, hydrochloric acid (4.5) + nitric acid (4.4) = 3 + 1, for some high-alloy steels] and heat gently until effervescence ceases. Decompose the carbides by the addition of nitric acid (4.4) drop by drop.

Continue heating until the surface of the solution calms down²⁾ and white fumes are just given off (controlling the temperature from 200 °C to 240 °C). Remove the flask from the heater, add 2 g of ammonium nitrate (4.1) immediately and shake the conical flask to remove nitrogen oxide. Nitrogen oxide must be eliminated thoroughly by blowing with a pipette or by adding 0,5 g to 1,0 g of urea (4.2). Wait for 1 min to 2 min. Cool the solution to 80 °C to 100 °C.

7.2.2 Titration

7.2.2.1 Visual titration

Add 60 ml of sulfuric acid (4.7) to the test solution (7.2.1) and mix. Make up the volume to approximately 150 ml and cool to room temperature.

Titrate the solution with the ferroammoniumdisulfate solution (4.11) until the end point is approached. Add 2 drops of N-phenylanthranilic acid (4.8). Continue the titration until the purplish red colour of the solution just disappears. Record the volume, V_3 , of the ferroammoniumdisulfate solution (4.11) added.

7.2.2.2 Potentiometric titration

Transfer the test solution (7.2.1) to a 400 ml beaker. Add 60 ml of sulfuric acid (4.7) and mix. Make up the volume to approximately 150 ml and cool to ambient temperature.

Place the beaker containing the solution on the magnetic stirrer and start it.

Immerse the indicator and reference electrodes [5 a) and 5 b)] or a redox electrode in the solution. Titrate slowly with the ferroammoniumdisulfate solution (4.11) until the end point is approached. Continue the titration in 0,05 ml or one drop increments, and record the volume added and potential readings when equilibrium is reached after each incremental addition. Continue the titration through the end point. Determine the end point by the titration curve or the first derivative of the potential difference divided by the first derivative of the volume of titrant (dE/dV). Record the end-point volume, V_4 , of the ferroammoniumdisulfate solution (4.11).

7.2.3 Theoretical correction of vanadium and cerium

For the samples containing vanadium and/or cerium, the mass fraction of manganese shall be corrected on the following theoretical basis.

Manganese, percent = vanadium, percent $\times 1,08$; manganese, percent = cerium, percent $\times 0,4$.

The mass fraction of vanadium may also be determined by the procedures specified in ISO 4942, ISO 4947 or ISO 9647 and the corresponding mass fraction shall be subtracted from the raw mass fraction of manganese.

8 Expression of results

8.1 Method of calculation

8.1.1 Visual titration

The mass fraction of manganese in the sample, w_{Mn} , expressed as a percentage, is given by the equation:

$$w_{Mn} = \frac{c \times (V_3 - V_0) \times 54,94}{m_0 \times 1\,000} \times 100 - 1,08 \times w_V - 0,4 \times w_{Ce}$$

where

- c is the concentration, in moles per litre, of the ferroammoniumdisulfate solution (4.11);
- V_0 is the volume, in millilitres, of the ferroammoniumdisulfate solution (4.11) for correction of N-phenylanthranilic acid;
- V_3 is the volume, in millilitres, of the ferroammoniumdisulfate solution (4.11) required to titrate manganese, vanadium and cerium;
- m_0 is the mass, in grams, of the test portion;
- 54,94 is the molar mass, in grams per mole, of manganese;
- w_V is the mass fraction of vanadium in the sample, expressed as a percentage;
- w_{Ce} is the mass fraction of cerium in the sample, expressed as a percentage.

8.1.2 Potentiometric titration

The mass fraction of manganese in the sample, w_{Mn} , expressed as a percentage, is given by the equation:

$$w_{\text{Mn}} = \frac{c_1 \times V_4 \times 54,94}{m_0 \times 1\,000} \times 100 - 1,08 \times w_{\text{V}} - 0,4 \times w_{\text{Ce}}$$

where

- c_1 is the concentration, in moles per litre, of the ferroammoniumdisulfate solution (4.11);
- V_4 is the volume, in millilitres, of the ferroammoniumdisulfate solution (4.11) required to titrate manganese, vanadium and cerium;
- m_0 is the mass, in grams, of the test portion;
- 54,94 is the molar mass, in grams per mole, of manganese;
- w_{V} is the mass fraction of vanadium in the sample, expressed as a percentage;
- w_{Ce} is the mass fraction of cerium in the sample, expressed as a percentage.

8.2 Precision

A planned trial of this method was carried out by 10 laboratories, at 7 levels of manganese; each laboratory making three determinations of mass fraction of manganese at each level.

NOTE 1 Two of the three determinations were carried out under repeatability conditions as defined in ISO 5725-1; i.e. one operator, same apparatus, identical operating conditions, same calibration, and a minimum period of time.

NOTE 2 The third determination was carried out at a different time (on a different day) by the same operator as in Note 1, using the same apparatus with a new calibration.

The test samples used are listed in Table A.1. The results obtained were treated statistically in accordance with ISO 5725-1, ISO 5725-2 and ISO 5725-3.

The data obtained showed a logarithmic relationship between the mass fraction of manganese and repeatability (r) and reproducibility (R and R_w) of the test results (see Note 3) as summarized in Table 2. The graphical representation of the data is shown in Annex B.

NOTE 3 From the two values obtained on day 1 and the value obtained on day 2, the repeatability limit (r) and reproducibility limit (R and R_w) were calculated using the procedure specified in ISO 5725-3.

Table 2 — Results for repeatability limit and reproducibility limits

Mass fraction of manganese %	Repeatability limit r	Reproducibility limits	
		R_w	R
2,00	0,023 2	0,035 6	0,067 8
5,00	0,041 3	0,061 3	0,131 2
10,00	0,063 7	0,092 6	0,216 4
12,00	0,071 4	0,103 3	0,246 8
15,00	0,082 2	0,117 9	0,289 9
20,00	0,098 4	0,139 9	0,356 7
22,00	0,104 5	0,148 1	0,382 1
25,00	0,113 2	0,159 8	0,419 0

9 Test report

The test report shall include the following information:

- the method used by reference to this International Standard;
- all information necessary of the identification of the sample, the laboratory and the data of analysis;
- the results and the form in which they are expressed;
- any unusual features noted during the determination;
- any operation not specified in this International Standard, or any optional operation which may have influenced the results.

Annex A (informative)

Additional information on the international cooperative test

The test samples used are listed in Table A.1. Detailed results for the mass fraction of manganese obtained in international cooperative tests are shown in Table A.2.

Table A.2 was derived from the results of international analytical trials carried out in 2006 on steel samples in 5 countries involving 10 laboratories.

The results of the trials were reported. The precision data are presented in graphical form in Annex B.

Table A.1 — Test samples used

Sample No.	No. of certified reference material	Chemical composition									
	(CRM)										
	Cr Ni Mo	C	Si	Mn	P	S					
		V	Cu								
1	GBW 01301	0.9	0.06	2.09	0.05	0.03	0.1	0.08			0.2
2	GBW 01657	0.07	0.5	4.76	0.03	0.01	11.5	4.5	3.1	0.02	0.1
3	YSBC 11301-93	0.06	0.9	10.03	0.02	0.003	18	5.7			
4	YSBC 11315-94	1.2	0.6	12.61	0.08	0.007	0.2	0.1			
5	BH1004-1	0,06	0,6	17,22	0,09	0,008	9,3				
6	BH 0227	0,2	0,2	22,44	0,02	0,001	0,02	0,003			Al 2,2


Table A.2 — Detailed results obtained in international cooperative test

No.	Sample	Mass fraction of manganese			Precision data		
		Certified value	%		Repeatability limit r	Reproducibility limits	
			Found \bar{w}_{Mn1}	Found \bar{w}_{Mn2}		R_W	R
1	GBW 01301	2,09	2,087 9	2,088 9	0,0202 64	0,034 535	0,072 097
2	GBW 01657	4,76	4,753 0	4,752 3	0,0563 80	0,063 467	0,113 486
3	YSBC 11301-93	10,03	10,081 6	10,079 9	0,0545 82	0,082 630	0,250 511
4	YSBC 11315-94	12,61	12,654 9	12,658 5	0,0600 17	0,118 712	0,263 062
5	BH1004-1	17,22	17,214 8	17,227 6	0,1309 46	0,164 007	0,284 362
6	BH 0227	22,44	22,349 1	22,362 8	0,0870 42	0,116 929	0,398 643
7	a	29,17 ^a	29,084 4	29,091 7	0,1239 65	0,146 246	0,505 787
\bar{w} general mean within a day \bar{w}_{Mn1}							
\bar{w} general mean over several days \bar{w}_{Mn2}							
a When the international cooperative test started, the scope of the mass fraction of manganese in the working draft specified 2 % to 30 %. Since there is no certified reference material (CRM) available for the level of 30 % (mass fraction of Mn), CRM BH0227 was used as two samples: one at the level of 22,44 % (mass fraction of Mn), another at the level of 30 % (mass fraction of Mn) by weighing 0,13 g, which is more than the normal, but being calculated as 0,1 g. In this line, the certified value, 29,17 % (mass fraction of Mn), is calculated by 22,44 % (mass fraction of Mn) times 1,3.							

According to the TC 17/SC 1 Resolution on October 18-20, 2006, the scope was changed to the mass-fraction range of 2 % to 25 %, and the data of sample No. 7 was removed from the statistical calculation of precision data.

Annex B (informative)

Graphical representation of precision data

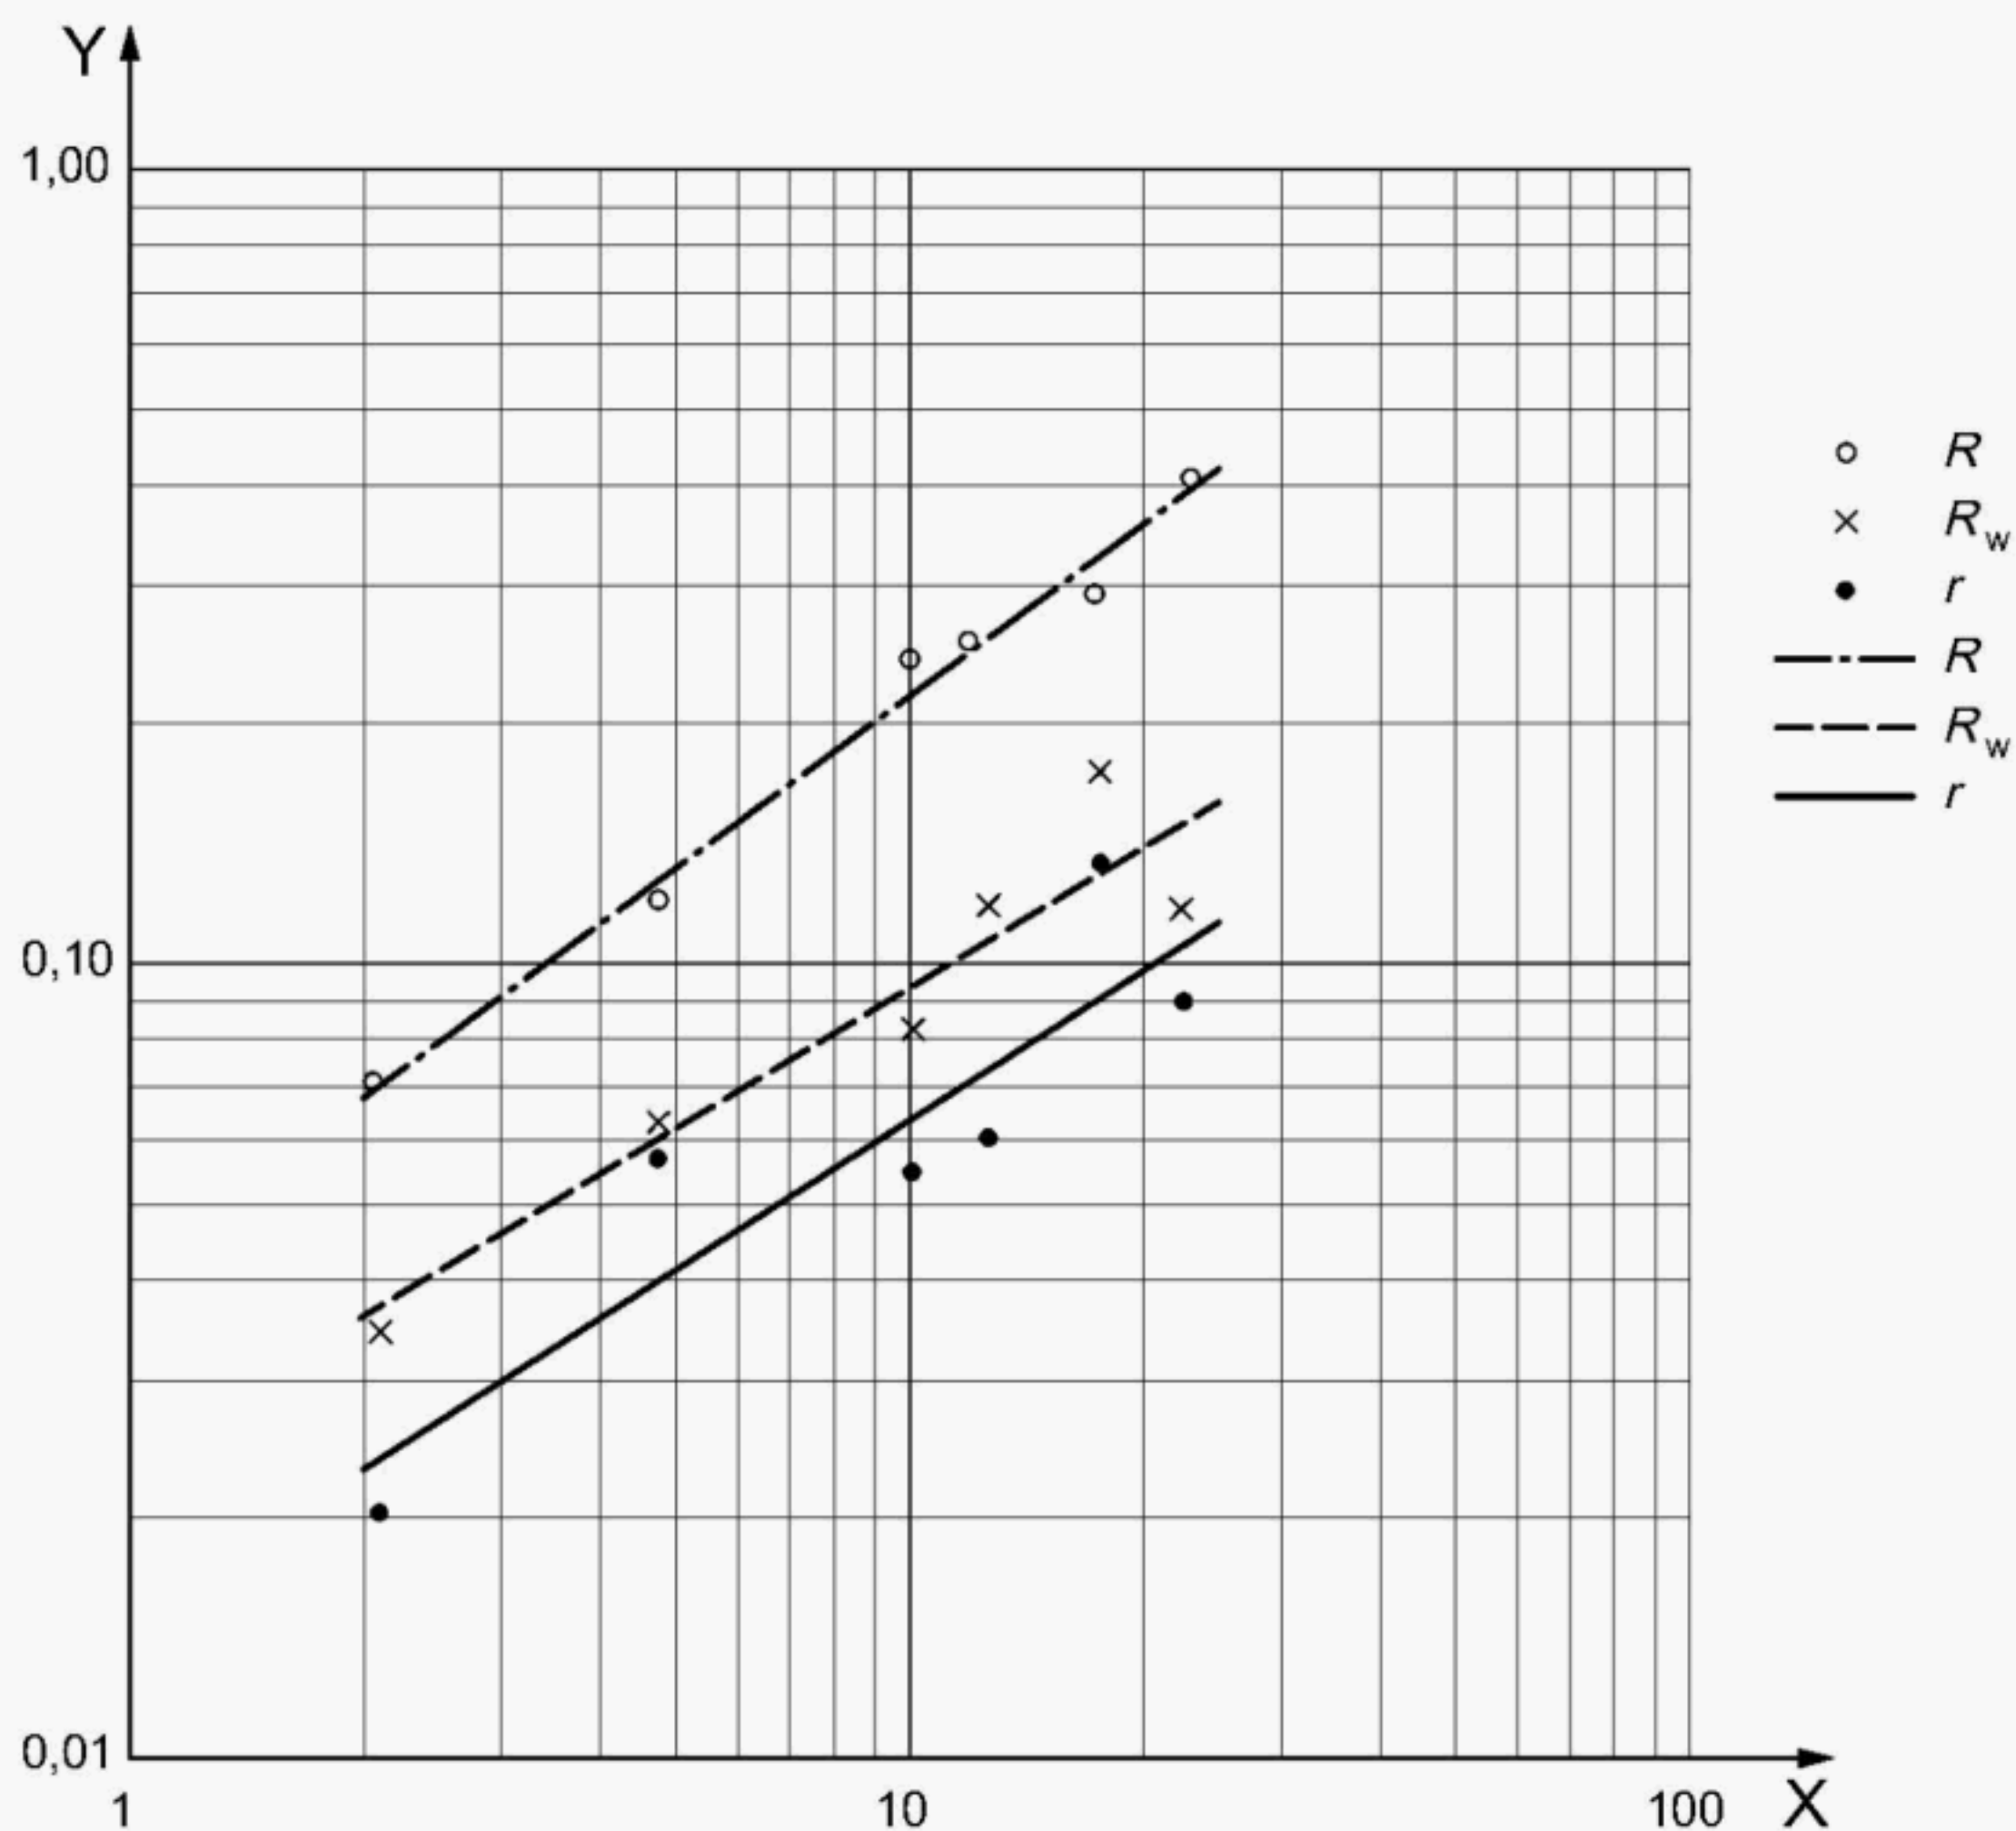

Key

X mass fraction of manganese, expressed as a percentage

Y precision of mass fraction, expressed as a percentage

$$\lg r = 0,627\,4 \lg \bar{w}_{\text{Mn}} - 1,823\,1$$

$$\lg R_w = 0,594\,8 \lg \bar{w}_{\text{Mn}} - 1,628\,0$$

$$\lg R = 0,7213 \lg \bar{w}_{\text{Mn}} - 1,386\,1$$

where w_{Mn} is the average mass fraction of manganese obtained from the three determinations in each laboratory.

Figure B.1 — Logarithmic relationship between mass fraction of manganese, w_{Mn} , and repeatability limit, r , and reproducibility limits, R_w and R

Bibliography

- [1] ISO 385, *Laboratory glassware — Burettes*
- [2] ISO 5725-1, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*
- [3] ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*
- [4] ISO 5725-3, *Accuracy (trueness and precision) of measurement methods and results — Part 3: Intermediate measures of the precision of a standard measurement method*

100

BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: orders@bsigroup.com You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: info@bsigroup.com

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: membership@bsigroup.com

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: copyright@bsigroup.com

BSI Group
Headquarters 389
Chiswick High Road,
London, W4 4AL, UK
Tel +44 (0)20 8996 9001
Fax +44 (0)20 8996 7001
[www.bsigroup.com/
standards](http://www.bsigroup.com/standards)

